



PGT[®]120.COM Data Terminal 2 (Part No.: 7100.PGT120.COM.DT)


The "Data Terminal 2", is a modular system for recording and processing Personnel Grounding Tester's test data. A basic system consists of: PGT120.COM (1) and Data Terminal (2). Test data can be stored for one month inside the device. The data can be retrieved by a web browser from any computer when connected to a network.

Test data can be imported to Time Attendance or Access Control systems via network interface.

Remote PC functions when connected to network:

- List of measurement data with coloured marking of failed tests
- Printed test results list
- WEB-interface for easy configuration
- German and English support

Overview

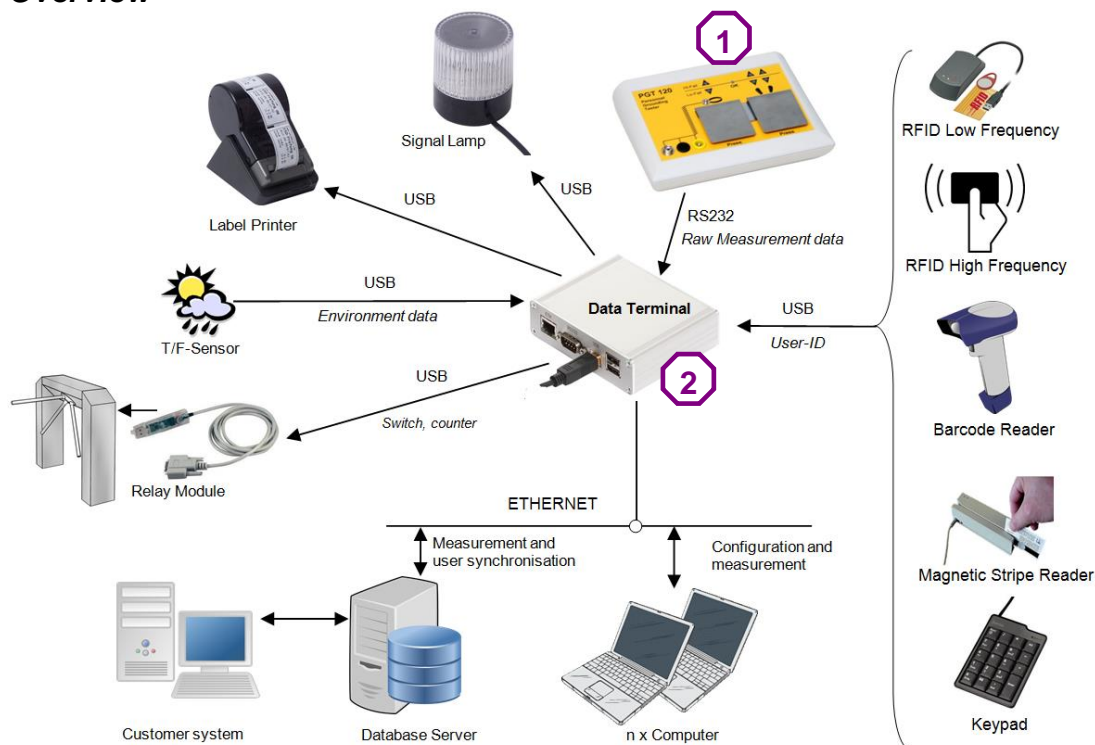



Certified by DQS
ISO 9001:2008




Wolfgang Warmbier[®]
Systeme gegen Elektrostatik

◆ Untere Gießwiesen 21 ◆ 78247 Hilzingen ◆ Tel.: +49-7731-86880 ◆ Fax: +49-7731-868830

Interface Connection Example

Two USB ports are available on the Data Terminal. For multiple extensions use a USB-HUB as distributor.

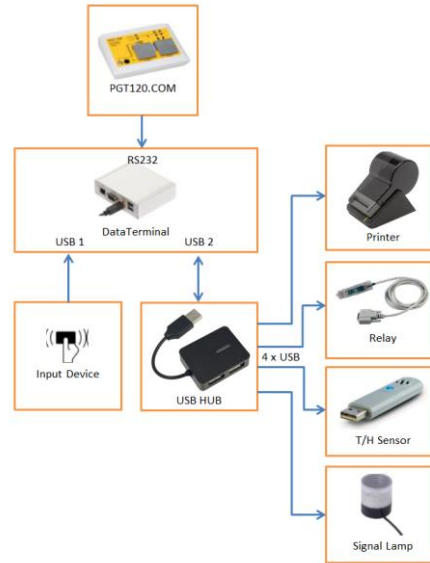

Measurement

Data Terminal - Mozilla Firefox

http://192.168.1.1/cgi-bin/pgt120-web.cgi?func=measure&

PGT120.COM Data Terminal - Measurement

History Sysinfo Configuration Logout

Date	Time	Shoe left	Shoe right	Wrist strap	Result	ID	Temp.	RH
2011-02-04	13:37	97.1 MΩ	20.2 MΩ		UserID missing		26.0°C	31.0%
2011-02-04	13:37	58.3 MΩ	21.1 MΩ		UserID missing		26.0°C	31.0%
2011-02-04	13:35			2.6 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			2.5 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			2.5 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	21.4 MΩ	27.7 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	23.1 MΩ	27.4 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	25.3 MΩ	27.3 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	24.4 MΩ	26.1 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			3.3 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			2.9 MΩ	UserID missing		26.1°C	30.5%
2011-02-04	13:34			2.8 MΩ	OK	15E8716D	26.1°C	30.5%
2011-02-04	13:34	23.8 MΩ	25.6 MΩ		OK	15E8716D	26.1°C	30.5%
2011-02-04	13:34	23.8 MΩ	26.4 MΩ		OK	15E8716D	26.1°C	30.5%
2011-02-04	13:34	25.9 MΩ	28.3 MΩ		UserID missing		26.1°C	30.5%
2011-02-04	13:24	21.6 MΩ	19.3 MΩ		OK	15E8716D	25.9°C	30.5%
2011-02-04	13:24	23.6 MΩ	20.4 MΩ		UserID missing		25.9°C	30.5%
2011-02-04	11:51	23.4 MΩ	23.3 MΩ		OK	A58FF340	25.4°C	30.5%
2011-02-04	11:51			2.4 MΩ	OK	A58FF340	25.4°C	30.5%
2011-02-04	11:51	23.7 MΩ	25.8 MΩ	2.2 MΩ	OK	A58FF340	25.4°C	30.5%
2011-02-04	11:50	25.7 MΩ	28.5 MΩ		OK	15E8716D	25.4°C	30.5%
2011-02-04	11:50	26.3 MΩ	27.6 MΩ		OK	15E8716D	25.4°C	30.5%
2011-02-04	11:50				Button released too early	15E8716D	25.4°C	30.5%
2011-02-04	11:50			2.3 MΩ	OK	15E8716D	25.4°C	30.5%
2011-02-04	11:50	25.9 MΩ	26.5 MΩ		OK	15E8716D	25.4°C	30.5%

Supplied with:

- Data Terminal
- Power supply
- User's manual (German / English)

*PGT120.COM must be ordered separately
Part.-No. 7100.PGT120.COM*



▶ 1 year limited warranty